



BOTTLE TOP DISPENSER

OPERATING MANUAL

TABLE OF CONTENTS*

Intended Use of the Instrument	3
Safety Instructions	3
Functions and Limitations of Use	4
Operating Exclusions	4
Storage Conditions	5
Chemical Resistance	5
List of Reagents	6
First Steps	10
Assembly	10
Priming	11
Dispensing	12
Error Limits	13
User Calibration Procedure	13
Maintenance/Cleaning	14
Dis-assembling the dispenser for cleaning and servicing	15
Autoclaving	17
Troubleshooting	18

**Clicking on the page numbers will take you directly to the corresponding section.*

INTENDED USE OF THE INSTRUMENT

The Dispenser is a general purpose laboratory instrument intended for use in laboratories for dispensing reagents and chemicals which are compatible with the instrument (see page 25).

SAFETY INSTRUCTIONS

This instrument may sometimes be used with hazardous materials, operations and equipments. It is beyond the scope of this manual to address all of the potential risks associated with its use in such applications. It is the responsibility of the user of this instrument to consult and establish appropriate safety and health practice and determine the applicability of regulatory limitations prior to use.

Please read the following carefully!

- Every user must read and understand this operating manual before operation
- Follow general instructions for hazard prevention and safety instructions
e.g. wear protective clothing, eye protection and gloves
- Observe all specifications provided by reagent manufacturers
- When dispensing inflammable media, make sure to avoid the built up of static charge, e.g. do not dispense into plastic vessels do not wipe instruments with a dry cloth
- Use the instrument only for dispensing liquids, with strict regard to the defined limitations of use and operating limitations, (see page 23). If in doubt, contact the manufacturer or supplier
- Always use the instrument in such a way that neither the user nor any other person is endangered. When dispensing, the discharge tube must always point away from you or any other person. Avoid splashes. Only dispense into suitable vessels
- Never press down the piston when the discharge tube closure is attached
- Never remove the discharge tube while the dispensing cylinder is filled
- Reagents can accumulate in the cap of the discharge tube. Thus, it should be cleaned regularly
- Never carry the mounted instrument by the cylinder sleeve or the valve block. Breakage or loosening of the cylinder may also lead to personal injury from chemicals
- Never use force on the instrument. Use smooth gentle movements to operate the piston upwards and downwards. Use only original manufacturer's accessories and spare parts
- Do not attempt to make any technical alterations. Do not dismantle the instrument any further than is described in the operating manual
- Always check the instrument for visual damage before use
- If there is a sign of a potential malfunction (e.g. piston difficult to move, sticking valve or leakage). immediately stop dispensing. Consult the 'Troubleshooting' section of this manual and contact the manufacturer if needed, (see page 37)

FUNCTIONS AND LIMITATIONS OF USE

The LABSOLUTE® bottle top dispenser is designed for dispensing liquids directly from the reservoir bottle. The instrument is calibrated according to the requirements of the DIN EN ISO 8655-5. When the instrument is correctly used, the dispensed liquid comes into contact with only the following chemically resistant materials: PTFE, FEP and Borosilicate glass.

LIMITATIONS OF USE:

This instrument is designed for dispensing liquids, with the following physical limits:

- Use temperature from +15°C to +40°C (from 59°F to 104°F) of instrument and reagent
- Vapor pressure up to max. 600 mbar. Aspirate slowly above 300 mbar, in order to prevent the liquid from boiling
- Kinematic viscosity 500 mm²
(dynamic viscosity [mPas] = kinematic viscosity [mm²/s] x density [g/cm³])
- Density: up to 2.2 g/cm³

OPERATING LIMITATIONS:

Liquids, which form deposits may make the piston difficult to move or may cause jamming (e.g. crystallizing solutions or concentrated alkaline solutions). If the piston becomes difficult to move, the instrument should be cleaned immediately. (see page 33) When dispensing inflammable media, make sure to avoid buildup of static charge, e.g. do not dispense into plastic vessels, do not wipe instrument with a dry cloth.

The Dispenser is designed for general laboratory applications and complies with the relevant standards, e.g. DIN EN ISO 8655. Compatibility of the instrument for a specific application (e.g. trace material analysis, food sector etc.) must be checked by the user. Certificates for specific applications, e.g. for production and administration of food, pharmaceuticals and cosmetics are not available.

OPERATING EXCLUSIONS

Never use with:

- Liquids attacking FEP, PFA and PTFE (e.g. dissolved sodium azide*)
- Liquids attacking borosilicate glass (e.g. hydrofluoric acid)
- Hydrochloric acid > 40%; Tetrahydrofuran; Trifluoroacetic acid
- Explosive liquids (e.g. carbon disulfide)
- Suspensions (e.g. of charcoal) as solid particles may clog or damage the instrument
- Liquids attacking PP (cap)

* Dissolved sodium azide permitted up to a concentration of max. 0.1 %

STORAGE CONDITIONS

Store the instrument and accessories only in clean conditions in a cool and dry place.

Storage temperature: from -20°C to +50°C (from -4°F to 122°F)

CHEMICAL RESISTANCE

Chemicals from A to Z

The following list includes most frequently used chemicals. It provides useful information for the safe and adequate use of LABSOLUTE® bottle top dispenser. However, safety precautions and recommendations in operating instructions must be followed carefully.

Code explanations

A = Good resistance

B = Acceptable with limitations

C = Not recommended

1 = Acid vapours (better resistance with lower concentration).

(do not leave instrument on bottle.)

2 = Risk of damage, softening or discoloration of external parts through vapours.

(do not leave instrument on bottle.)

3 = Chemical degradation of glass parts (plunger/barrel).

LIST OF REAGENTS

A			
Acetaldehyde (Ethanal)	A	Butanol	A
Acetic acid 96 %	A	Butanone (MEK)	B/2
Acetic acid 100 % (glacial)	B/2	Butyl acetate	B/2
Acetic anhydride	B/2	Butyl methyl ether	B/2
Acetone (Propanone)	B/2	Butylamine	B/2
Acetonitrile (MECN)	A	Butyric acid	B/2
Acetophenone	B/2	Butyric acid	B/4
Acetyl Chloride	B/2	C	
Acetylacetone	A	Calcium carbonate	A
Acrylic acid	A	Calcium chloride	A
Acrylonitrile	B/2	Calcium hydroxide	A
Adipic acid	A	Calcium hypochlorite	A
Allyl alcohol	A	Carbon disulfide	B/2
Aluminum chloride	A	Carbon tetrachloride	B/2
Amino acids	A	Chlorine dioxide	B/2
Ammonia 20 %	B/2	Chlorine water	B/2
Ammonia 20–30 %	B/2	Chloro naphthalene	B/2
Ammonium chloride	A	Chloroacetaldehyde 45 %	A
Ammonium fluoride	A	Chloroacetic acid	A
Ammonium molybdate	A	Chloroacetone	B/2
Ammonium sulfate	A	Chlorobenzene	B/2
Amyl alcohol (Pentanol)	A	Chlorobutane	B/2
Amyl chloride (Chloropentane)	B/2	Chloroethanol	B/2
Aniline	A	Chloroform	B/2
Ascorbic acid	A	Nitro-hydrochloric acid (Aqua regia)	B/2
n-Amyl acetate	B/2	Chlorosulfonic acid	B/2
B		Chlorosulfuric acid 100 %	B/1/2
Barium chloride	A	Chromic acid 100 %	B/1/2
Benzaldehyde	A	Chromosulfuric acid 100 %	C/1/2
Benzene	B/2	Citric acid	A
Benzine	A	Copper fluoride	A
Benzoyl chloride	B/2	Copper sulfate	A
Benzyl alcohol	A	Cresol	A
Benzyl chloride	B/2	Cumene (Isopropylbenzene)	B/2
Bis(2-ethylhexyl) phthalate	B/2	Cyanoacrylate	A
Boric acid 10 %	A	Cyclohexane	B/2
Bromine	C/2	Cyclohexanone	B/2
Bromobenzene	B/2	Cyclopentane	B/2
Bromonaphthalene	A	D	
Butanediol	A	1,2-Diethylbenzene	B/2
		1,4-Dioxane (Diethylene dioxide)	B/2

1-Decanol	A	Hydrobromic acid	A
Decane	A	Hydrochloric acid 20 % (HCl)	A
Di-(2-ethylhexyl) peroxycarbonate	B/2	Hydrochloric acid 37 % (HCl)	B/1
Dibenzyl ether	B/2	Hydrofluoric acid (HF)	C/3
Dichloroacetic acid	A	Hydrogen peroxide	A
Dichlorobenzene	A	I	
Dichloroethane	A	Iodine	A
Dichloroethylene	B/2	Iodine bromide	C/2
Diesel oil (Heating oil)	A	Iodine chloride	C/2
Diethanolamine	A	Isoamyl alcohol	A
Diethylamine	B/2	Isobutanol	A
Diethylene glycol	A	Isooctane	A
Diethylether	B/2	Isopropanol	A
Dimethyl sulfoxide (DMSO)	B/2	Isopropyl ether	B/2
Dimethylaniline	A	Iso-propylamine	B/2
Dimethylformamide (DMF)	B/2	K	
E		Kerosene	A
Ethanol	A	L	
Ethanolamine	B/2	Lactic acid	A
Ether	B/2	M	
Ethyl acetate	B/2	2-Methoxyethanol	A
Ethylbenzene	B/2	Methanol	A
Ethylene chloride	B/2	Methoxybenzene (Anisol)	B/2
Ethylene diamine	A	Methyl benzoate	B/2
Ethylene glycol	A	Methyl chloride (Chloromethane)	B/2
F		Methyl ethyl ketone (MEK/Butanone)	B/2
Fluoroacetic acid	B/2	Methyl formate	A
Formaldehyde (Formalin)	A	Methyl iodide (Iodomethane)	B/2
Formamide	A	Methyl methacrylate (MMA)	B/2
Formic acid	A	Methyl propyl ketone (2-Pentanone)	A
G		Methyl tert-butyl ether	B/2
Gamma-butyrolactone	A	Methylene chloride (Dichloromethane) (DCM)	B/2
Gasoline	B/2	Methylpentanone	A
Glycerin <40 %	A	Mineral oil (engine oil)	A
Glycolic acid 50 %	A	Monochloroacetic acid	A
H		N	
Heating oil (Diesel oil)	A	Nitric acid 100 %	A
Heptane	A	Nitric acid 30–70 %	A
Hexane	A	Nitric acid dil. <30 %	A
Hexanoic acid	A	Nitrobenzene	B/2
Hexanol	A	Nitromethane	B/2
Hydriodic acid	B/2		

N-methyl-2-pyrrolidone (NMP)	A
O	
Octane	A
Octanol	A
Oil (vegetable, animal)	B/2
Oil of turpentine	B/2
Oleic acid	A
Oleum (Fuming Sulfuric Acid)	A
Oxalic acid	A
P	
Pentane	B/2
Peracetic acid	A
Perchloric acid 100 %	B/2
Perchloric acid diluted	A
Perchloroethylene	B/2
Petroleum	B/2
Petroleum ether/spirit	B/2
Phenol	A
Phenylethanol	B/2
Phenyldiazine	B/2
Phosphoric acid 100 %	A
Phosphoric acid 85 %	A
Piperidine	B/2
Potassium chloride	A
Potassium dichromate	A
Potassium dihydrogen phosphate	A
Potassium hydroxide	A
Potassium iodide	A
Potassium permanganate (persulfate)	A
Potassium peroxydisulfate	A
Potassium sulfate	A
Propionic acid (Propanoic acid)	A
Propylene glycol (Propane-1,2-diol)	A
Propylene oxide	A
Pyric acid (Trinitrophenol)	B/2
Pyridine	B/2
Pyruvic acid	A
Pyruvic acid	A
R	
Resorcin	A

S	
Salicylaldehyde	A
Scintillation fluid	A
Silver acetate	A
Silver nitrate	A
Sodium acetate	A
Sodium chloride (kitchen salt)	A
Sodium dichromate	A
Sodium fluoride	A
Sodium hydroxide 30 %	A
Sodium hypochlorite	A
Sodium thiosulfate	A
Sulfonitric acid 100 %	B/2
Sulfur dioxide	B/2
Sulfuric acid 100 %	B/2
Sulfuric acid <10 %	A
Sulfuric acid (10–75 %)	B/1
Sulfuric acid (Cold conc.)	A
Sulfuric acid (Hot conc.)	B/2
T	
1,1,2-Trichlorotrifluoroethane	B/2
Tartaric acid	A
Tetrachlorethylene	B/2
Tetrahydrofuran (THF)	B/2
Tetramethylammonium hydroxide	A
Toluene	B/2
Trichlorethylene	B/2
Trichloroacetic acid	B/2
Trichlorobenzene	B/2
Trichloroethane	B/2
Trichloromethane (Chloroform)	B/2
Triethanolamine	A
Triethylene glycol	A
Trifluoroacetic anhydride (TFAA)	B/2
Trifluoromethane (Fluoroform)	B/2
U	
Urea	A
X	
Xylene	B/2
Z	
Zinc chloride 10 %	A
Zinc sulfate 10 %	A



FIRST STEPS

Confirm that package includes: Bottle Top Dispenser, discharge tube, telescoping filling tube, calibration tool, different bottle adapters, a calibration certificate and this operation manual. All dispensers will have the following adapters : 28, 32, 38, 40 & 45 mm.

ASSEMBLY

Wear protective clothing, eye protection and gloves. Follow all Safety instruction and observe limitations of use and operating limitations. (see page 23)

1. Adjust length of telescoping inlet tube. The length of FEP inlet tubing provided should be adjusted to fit your particular reservoir. Longer length of inlet tube are available on request. (Fig. 1)
2. Fix the telescoping tube. (Fig. 2)
3. Choose the correct adapter for the bottle. The threaded platform base of dispenser has a 30 mm screw thread. Five adapters are supplied to suit containers with a 28, 32, 38, 40, 45 mm and 30 mm (inbuilt adapter) screw neck. (Fig. 3)
4. Fix the adapter. (Fig. 4)
5. Mount the dispenser: The assembled dispenser is screwed to the reservoir using gentle hand torque applied to the threaded platform base only. Removal should also be by means of hand torque applied to the same base. (Fig. 5)
6. Ready to Use.



Fig. 1



Fig. 2



Fig. 3



Fig. 4



Fig. 5

Do not operate the piston until the unit is safely and fully mounted on the reservoir bottle.

! Always wear protective gloves when touching the instrument or the bottle, especially when using dangerous liquids. When mounted to a reagent bottle, always carry the instrument as shown in the figure 5.

! Never press down the piston when the cap is on. Avoid splashing the reagent. The reagent can drip out from the discharge tube and cap. (Fig. 6)



PRIMING

Open the cap of the dispensing tube (Fig. 6). For safety hold the discharge tube orifice on the inner wall of a suitable receiving vessel.



1. Set valve to ‚Recirculate‘. (Fig. 7)

For priming gently pull up the piston approx. 30mm and push it down rapidly until the lower stop. Repeat this procedure 5 times (Fig. 8).



2. Turn valve to ‚Dispense‘. (Fig. 9)

To avoid splashes when priming hold the discharge tube on the inner wall of a suitable receiving vessel and dispense liquid to prime the discharge tube until it is bubble free, Wipe away any remaining drops from the discharge tube.



! Before using the instrument for the first time, ensure it is rinsed carefully and discard the first few samples dispensed. Avoid splashing.

DISPENSING

1. Volume Setting:

Volume Adjustment Knob

It is simple and easy to operate. There are two

positions of the knob as shown in Fig. 10a

Position 1: Locked Position

Position 2: Unlocked Position

Setting the Volume

Follow these simple steps:

- Turn the Knob from Position 1 to Position 2 by rotating it ANTI-CLOCKWISE as shown in Fig. 10b.
- The slider is now loose and can be moved up and down.
- Set your desired volume by aligning the pointer with the scale.
- To lock the set volume, turn the Knob from Position 2 to Position 1 by rotating it CLOCKWISE as shown in Fig. 10c .

2. Dispensing:

- Remove cap from the discharge tube (Fig. 11)
- When using the instrument (with recirculation valve) turn the valve to Dispensing (Fig. 12)
- Hold the discharge tube orifice on the inner wall of a suitable receiving vessel (Fig. 13)
- Gently lift the piston until the upper stop and then depress piston slowly and steadily with minimal force until the lower stop (Fig. 14)
- Wipe off the discharge tube against the inner wall of the receiving vessel
- Reattach cap to discharge tube (Fig. 15)

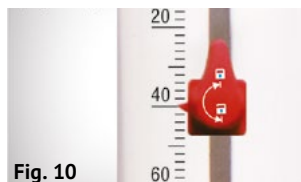


Fig. 10



Fig. 10a




Fig. 10b




Fig. 10c



Fig. 11



Fig. 12



Fig. 13



Fig. 14



Fig. 15

ERROR LIMITS

Error Limits related to the nominal capacity (= maximum volume) indicated on the instrument, are obtained when instrument and distilled water are equilibrated at ambient temperature (20°C/68°F). Testing takes place according to DIN EN ISO 8655-6 with a completely assembled instrument and with uniform and smooth dispensing.

Art. no.	Vol. Range	Increment	Specifications ISO 8655			
			Accuracy		CV	
			±%	± ml	±%	± ml
7.695 540	0.25–2.5 ml	0.05 ml	0.6	0.015	0.2	0.005
7.695 541	0.5–5 ml	0.1 ml	0.6	0.030	0.2	0.010
7.695 542	1–10 ml	0.2 ml	0.6	0.060	0.2	0.020
7.695 543	2.5–30 ml	0.5 ml	0.6	0.180	0.2	0.060
7.695 544	5–60 ml	1.0 ml	0.6	0.360	0.2	0.120
7.695 545	10–100 ml	2.0 ml	0.6	0.600	0.2	0.200

USER CALIBRATION PROCEDURE

Dispenser has been laboratory calibrated at its nominal volume. However, due to changes in environmental conditions and the viscosity of the media which you dispense, we recommend gravimetric testing every 3 months. Gravimetric volume testing according to DIN EN ISO 8655-6 (for measurement conditions, see 'Error Limits', page 32) is performed as follows:



Fig. 16



Fig. 17



Fig. 18

Re-Calibrate

1. Set the Dispenser to the nominal volume or any other volume which is most commonly used by you. (Fig. 16) Follow the common rules for calibration used in statistical quality control (ISO 8655/2). Set the volume and dispense five full volumes of distilled water at 20°C on Electronic Balance to establish the actual mean volume of liquid dispensed. If the gravitational average result varies from the volume displayed, you should re-calibrate the Dispenser.
2. For re-calibration pull the cap outwards to expose the Calibration nut. (Fig. 17)
3. Using the calibration tool, turn the calibration nut clockwise to reduce the volume and anticlockwise to increase the volume. Repeat this procedure till the desired volume is achieved on the electronic balance. (Fig. 18)

MAINTENANCE/CLEANING

The Dispenser should be cleaned in the following situations:

- Immediately when the piston is difficult to move
- Before changing the reagent. Prior to long term storage
- Prior to dismantling the instrument
- Prior to autoclaving
- Prior to changing the valve
- Regularly when using liquids which form deposits (e.g. crystallizing liquids)
- Regularly when liquids accumulate in the cap

All maintenance should be carried out wearing suitable eye protection and protective clothing. If in doubt, consult your safety officer.

1. Make sure that the Dispenser is completely empty.
2. Place the instrument into an empty sink together with its reservoir.
3. Unscrew the threaded platform base from the reservoir and lift the dispenser's intake tube carefully out of the reservoir, whilst tapping it against the reservoir's aperture to shake off any droplets from the intake tube.
4. Hold the dispense nozzle over the aperture of the reservoir and apply gentle piston strokes in order to return any contents into the reservoir.
5. Empty the instrument completely and flush thoroughly with distilled water.
6. If the piston barrel is still not completely clean, you need to disassemble the dispenser. Refer Disassembling procedure given below.



DIS-ASSEMBLING THE DISPENSER FOR CLEANING AND SERVICING

Procedure to disassemble the piston

1. Pull the cap outwards to expose the Calibration Nut (Fig. 19)
2. Unscrew the Calibration Nut with the help of calibration tool to disassemble the Piston and shaft out of the main housing. (Fig. 20)
3. After unscrewing pull out the shaft. (Fig. 21)
4. Rinse the piston and shaft with deionized water. (Fig. 22)
5. Clean the cylinder with a bottle-brush. If necessary carefully remove deposits at the edge of the glass cylinder. (Fig. 23)
6. Then flush all the parts of the instrument with deionized water. (Fig. 24)
7. Insert the piston completely into the cylinder and then reassemble the instrument using the calibration tool by screwing back the piston. (Fig. 25)
8. Snap back the cap to complete the assembly. (Fig. 26)



Procedure to dis-assemble the delivery pipe

1. Unscrew the chuck nut (Fig. 27) and pull out the delivery pipe. (Fig. 28)
2. Clean the delivery pipe with deionized water.



Procedure to re-assemble the delivery pipe

1. First push the delivery pipe into the lower housing till it stops going in further. (Fig. 29)
2. Screw the chuck nut to complete the assembly. (Fig. 30)





Fig. 31



Fig. 32



Fig. 33



Fig. 34



Fig. 35



Fig. 36

AUTOCLAVING

This instrument is autoclavable at 121 °C (250 °F) 1 bar absolute (15 psi) with a holding time of at least 15 minutes.

⚠ Only the piston needs to be removed for autoclaving the instrument.

Dis-assembling for Autoclaving

1. Pull the cap outwards to expose the Calibration Nut. (Fig. 31)
2. Unscrew the Calibration Nut with the help of calibration tool to dis-assemble the Piston and shaft out of the main housing. (Fig. 32)
3. After unscrewing pull out the shaft. (Fig. 33)
4. This is the piston-shaft sub-assembly. (Fig. 34)
5. Autoclave the two sub-assemblies at 121 °C and 15 psi pressure for 10–15 mins. (Fig. 35)

Re-assembling after Autoclaving

1. Insert the piston completely into the cylinder and then reassemble the instrument using the calibration tool by screwing back the piston. (Fig. 36)
2. Snap back the cap to complete the assembly. (Fig. 37)
3. Dispenser is now ready for use. Recalibration is required after autoclaving. (Fig. 38)



Fig. 37



Fig. 38

TROUBLESHOOTING

Trouble	Possible Cause	Solution
Piston difficult to move	Formation of crystals, dirty	Stop dispensing immediately. Loosen piston with circular motion, but do not disassemble. Follow all cleaning instructions. (See page 14)
Air bubbles appear in the instrument	Reagent with high vapor pressure has been drawn in too quickly	Slowly draw in reagent.
	The instrument has not been primed	Prime the instrument. (See page 11)
	Filling tube is loose or damaged	Push the filling tube on firmly. If necessary cut off approx. 1 cm of the tube at the upper end and then re-connect it or replace filling tube.
Dispensing not possible	Liquid reservoir is empty	Refill reservoir and prime unit.
	Too fast filling action	Fill and dispense slowly.
	Leaking Piston	Clean Piston (see page 14). If problem persists replace piston.
	Leaking discharge valve	Clean by flushing thoroughly with distilled water. (See page 14)
	Blocked Dispense nozzle	Disassemble the dispense nozzle and flush through with distilled water.
Wrong dispenser volume	Discharge valve stuck	Clean Unit by immersing valve assembly in distilled water. (See page 14)
	Instrument not calibrated	Follow steps of user calibration. (See page 13)
Barrel does not fill with liquid	Inlet tube not fitted firmly	Connect inlet tube correctly. (See page 10, Fig. 2)
Filling not possible	Volume adjustment to Minimum setting	Set to required volume. (See page 12)

Germany

Tel.: 0800 4393784
Fax: 0800 8443937
sales@thgeyer.de

Scandinavia

Tel.: +45 4630 0030
sales@thgeyer.dk

Tel.: +46 8 6030200
sales@thgeyer.se

Poland

Tel.: +48 2242764-64
sales@thgeyer.pl

Other countries

Tel.: +49 7159 1637-823
Fax: +49 7159 18417
sales@thgeyer.com

www.thgeyer.com

